USE:

1. This product is intended for use as a medical device to aid in the prevention and treatment of pressure ulcers and for general comfort.
2. Include skin inspections, proper nutrition, turning schedules and daily inflation checks as part of a balanced pressure area care management programme.

MAINTENANCE:

1. Products should be at normal room temperature before inflating. Store in room temperature of 13° C to 29° C.
2. Clean all EHOB products with soap and water. Products can be cleaned using a diluted bleach cleaning solution equal to or less than 20%. Products can be cleaned with non-invasive Clinell Universal medical wipes. Do not use cleaning solvents containing petroleum distillates. Refer to local infection control policy for cleaning/disinfection of mattresses. Do not wash or dry in institutional laundry. This product may be washed at home up to 40° C. Do not tumble dry. Proper product inflation and skin care protocol must be maintained to maximize the skin care management provided by these products.
3. Use facility procedure for disposing of product and packaging materials.

PLEASE READ:

1. An anti-microbial agent is blended within the material formula of the product.
2. This product has flame resistant qualities in accordance with BS 7175 Crib Test 5.
3. Do not use near open flame.
4. This product is not sterile and is not intended to be sterilized.
5. Keep packaging materials away from children.
6. Not made with natural rubber latex.
7. All EHOB products are backed by a limited warranty that varies in duration depending on the product. Products found defective in workmanship or materials will be replaced provided failure is not the result of abuse or misuse, alteration or modification, and occurs within the specified warranty period. Tampering with the product voids warranty. (Example: glue or any unauthorized patching device.) Please contact our customer service department for full details.

EHOB®
prevention • treatment • solutions

Innovation Rehab ltd
Unit 7, Septimus Buildings
Hawkfield Business Park
Whitchurch
Bristol
BS14 0BN
UK Sales/Customer Service
Ph: +44 0117 9640818
Web: www.ehob-europe.com
E-Mail: sales@innovationrehab.co.uk
ISO 9001:2008
U.S. Patent No. 9,301,866 - 4440
EU Patent No. 2,505,167 - 4440
Patent Pending - 4400, 4410, 4420, 4430

EHOB Heel Protectors - UK

Indications for use:

Heel and lower extremity protection and healing therapy up to and including Stage IV pressure ulcers and deep tissue injury protection.

Product	Calf Size	Model	Warranty
Heel Elevator Custom - Petite/TPU	25 cm – 29 cm	4400	1 Year
Heel Elevator Custom - Standard/TPU	30 cm – 36 cm	4410	1 Year
Heel Elevator Custom - Extra/TPU	37 cm – 46 cm	4420	1 Year
Heel Elevator Custom - TPU	One size fits most	4430	1 Year
Heel Elevator Original - TPU	One size fits most	4440	1 Year

For Product Ordering Codes, contact your sales representative or UK Sales Centre, +44 0117 9640818

Proper product inflation and skin care protocol must be maintained to maximize the benefits of these products. Skin inspection, hand checks and turning schedules are vital to your skin care programme.

Daily hygiene consists of removing the product and washing, drying and inspecting the patient's foot and leg.

Directions for Use and Special Considerations

Set the heel of the foot in the product first, keeping the heel and foot perpendicular to the product. Close the foot gate first.

After the leg is placed in the product, secure the buttons on the straps for the patient's leg.

Secure the buttons on the straps across the patient's foot.

Note: Tubing from athrombic compression devices (sequential compression devices) should be brought through the boot in areas that will avoid pressure points on the leg and foot.

Caution:

- Designed for non-ambulatory use.
- Anti-embolism stockings, dressings or cotton socks should not interfere with product effectiveness.

Check that the patient's heel is offloaded from the surface of the bed.

Insert hand along the side of the foot, down toward the malleolus. The fingers should slide into the opening without difficulty.

To protect patients who 'dig' their heels, release the heel cushion, bring the strap up to the end of the heel flap and reseal. This feature may also be used when the wearer sits in a chair.

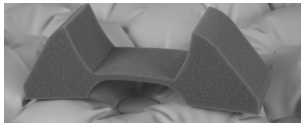

Anti-Rotation Wedge sold separately.